


PRIOR ART

FIG. 1

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR


Brauker, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.011A

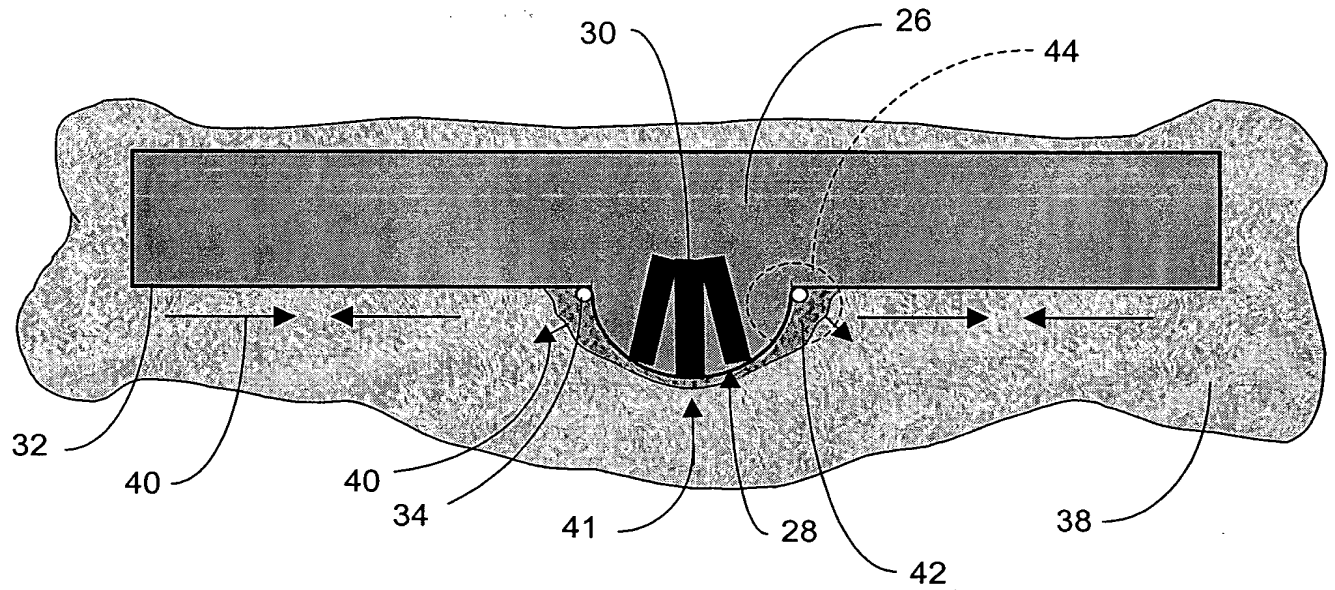


PRIOR ART

FIG. 2A

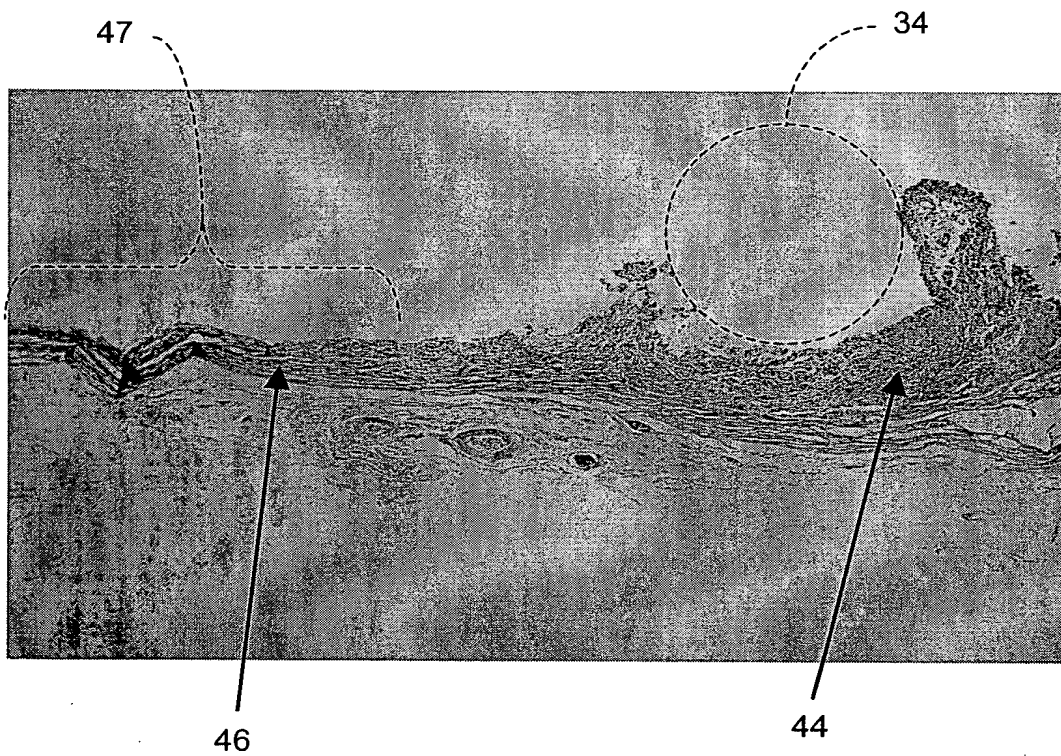

PRIOR ART

FIG. 2B

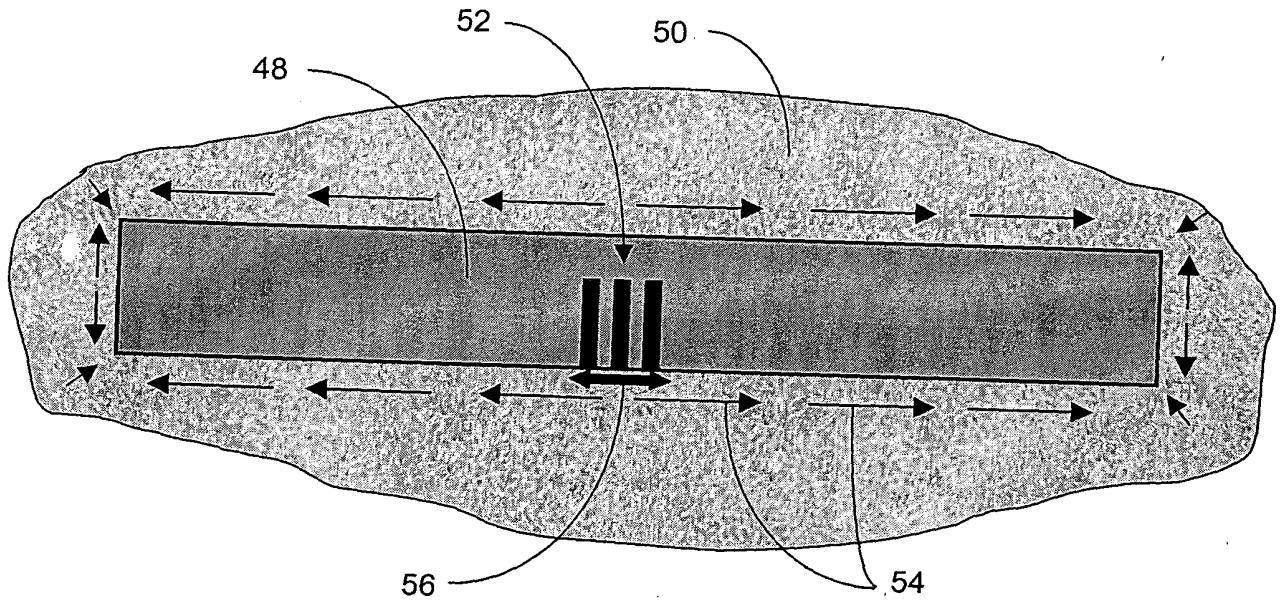

PRIOR ART

FIG. 3A

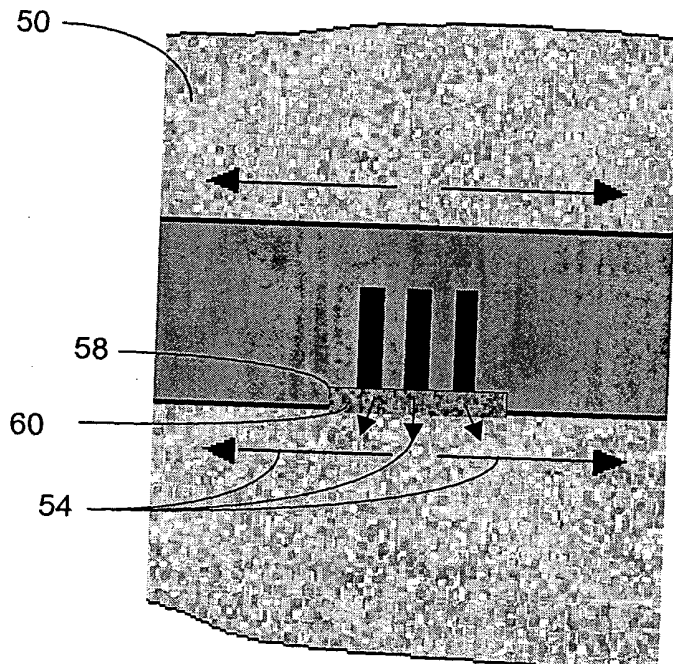


FIG. 3B  
PRIOR ART

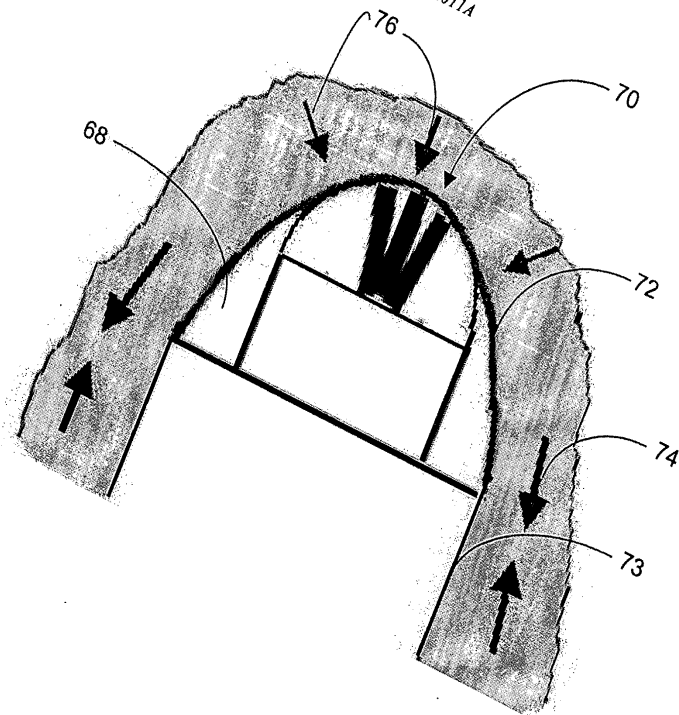


FIG. 4

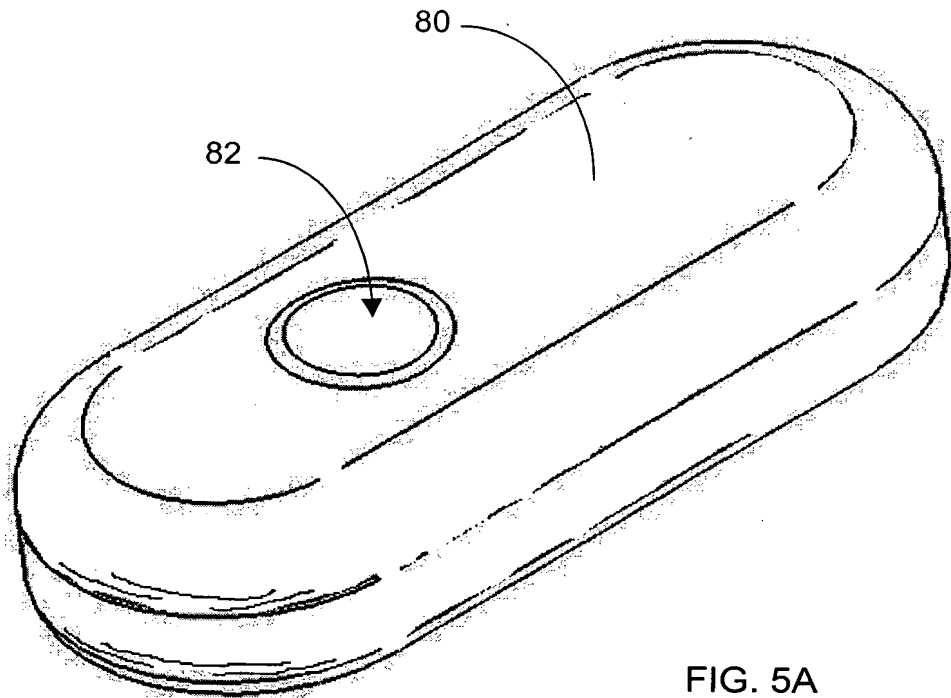


FIG. 5A

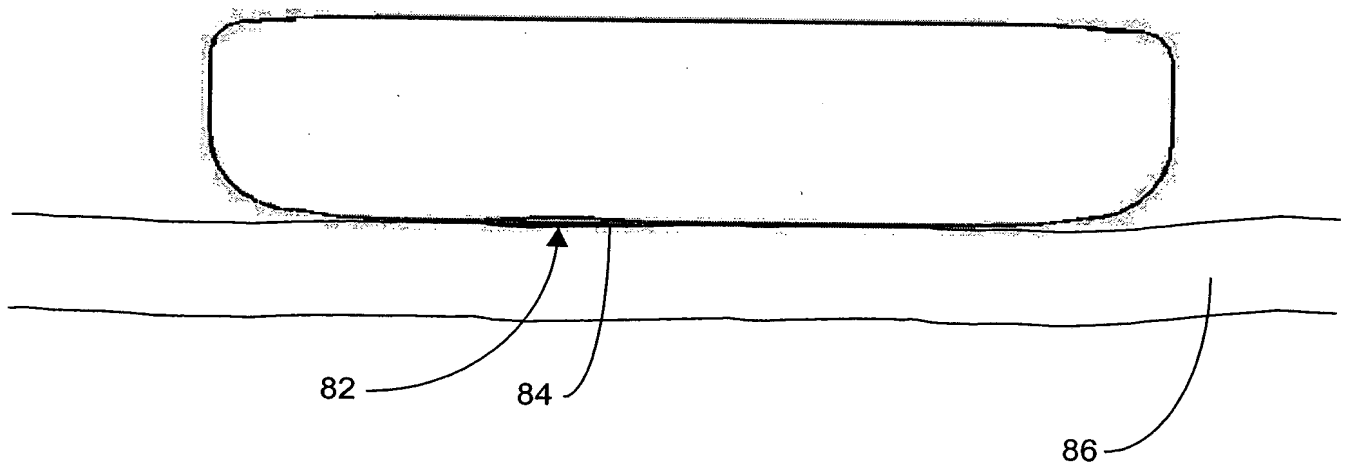


FIG. 5B

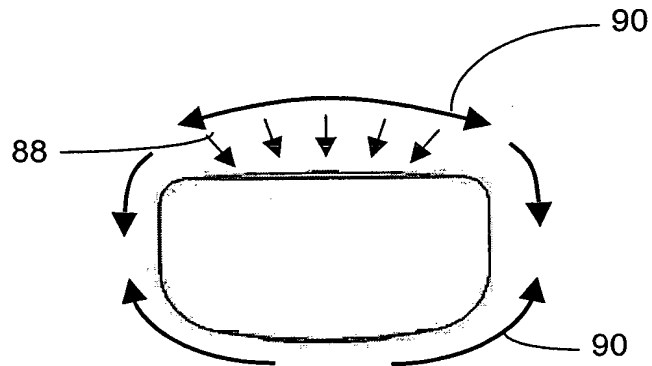


FIG. 5C

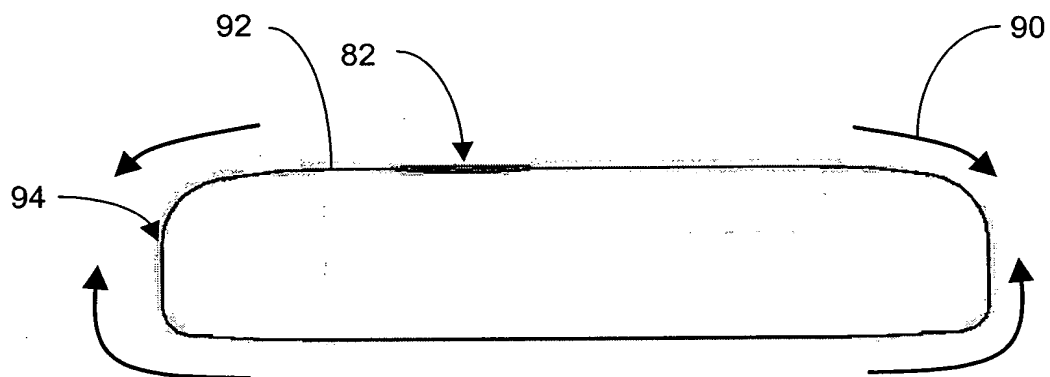


FIG. 5D

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown

Atty Docket: DEXCOM.011A

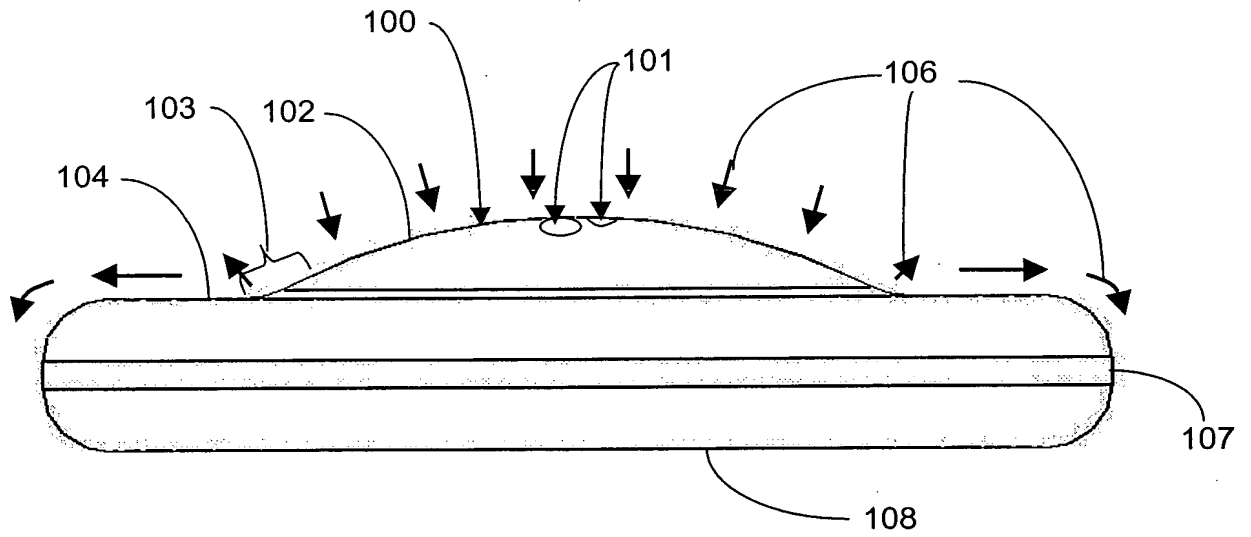


FIG. 6

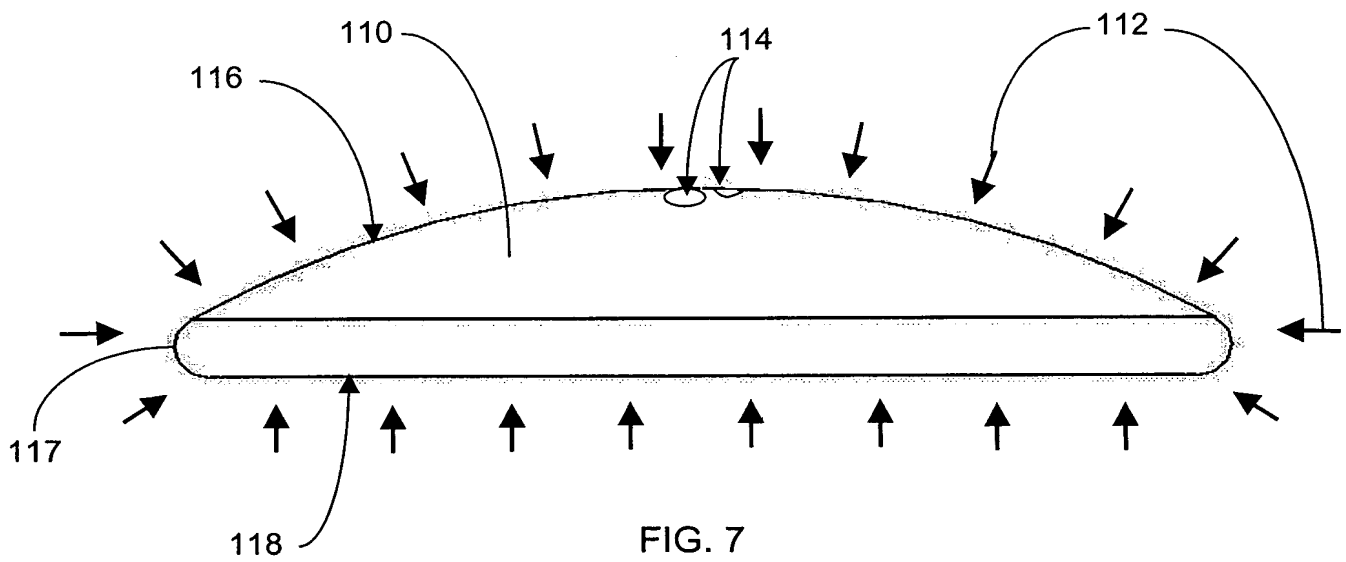


FIG. 7

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

*Brauker, et al.*

*Appl. No.: Unknown*

*Atty Docket: DEXCOM.011A*

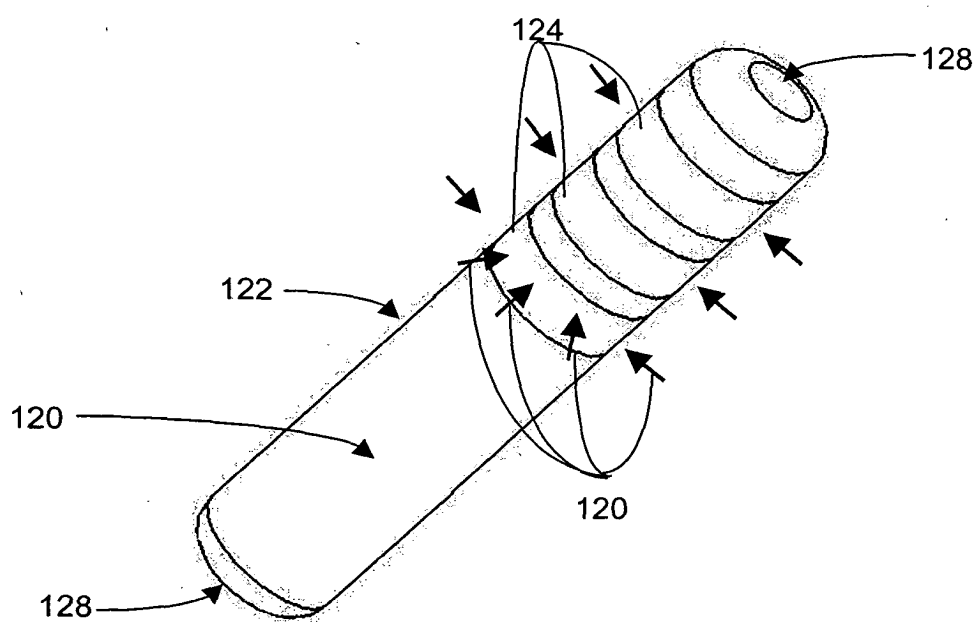


FIG. 8



OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.011A

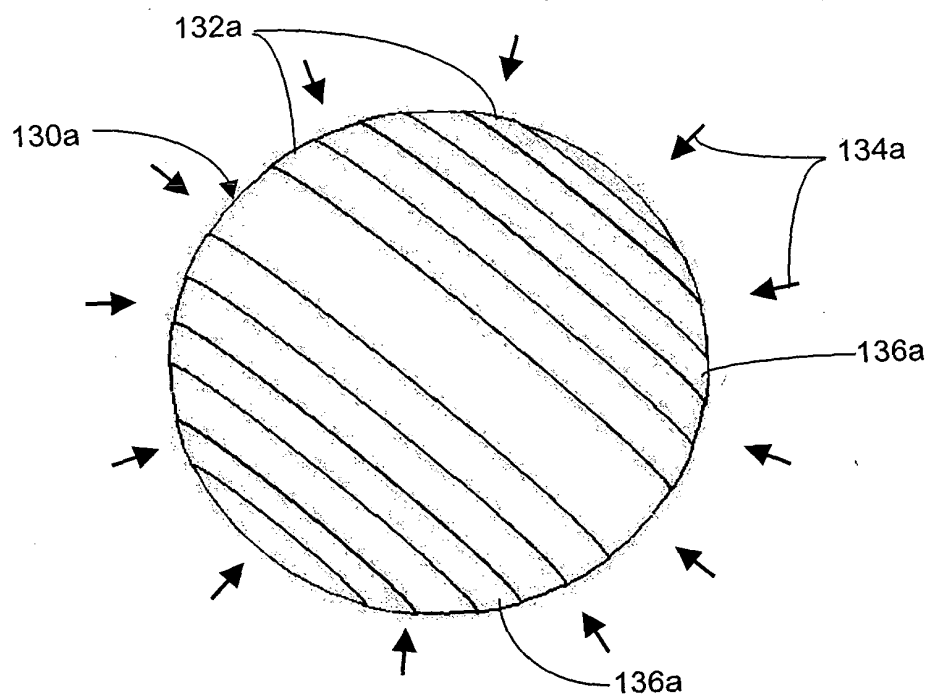


FIG. 9A

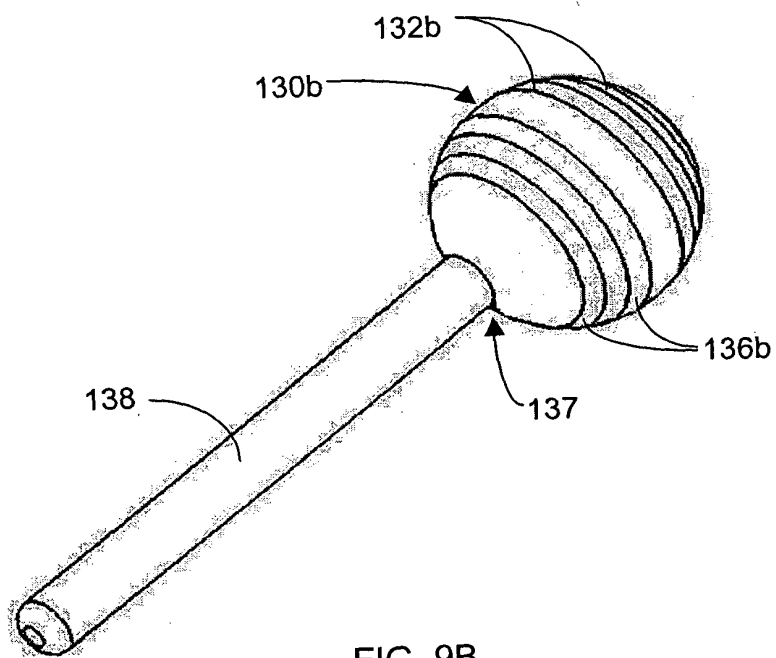


FIG. 9B

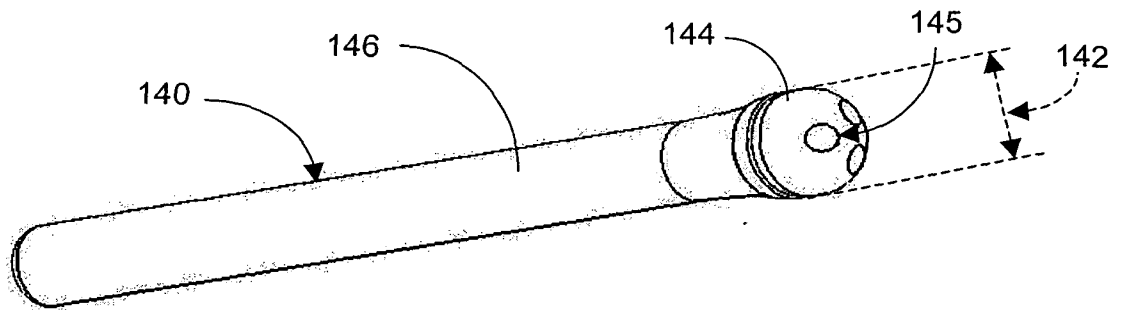


FIG. 10A

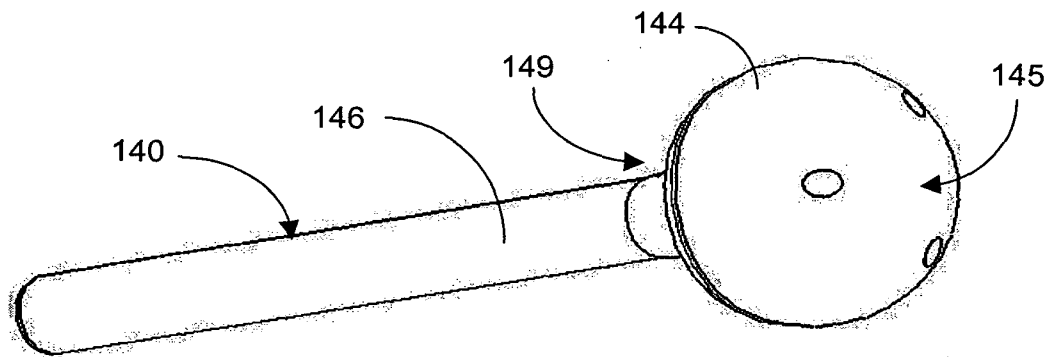


FIG. 10B

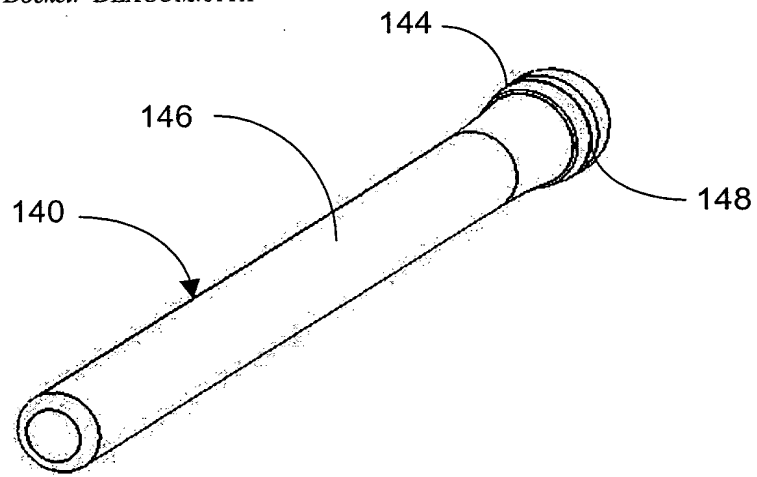


FIG. 10C

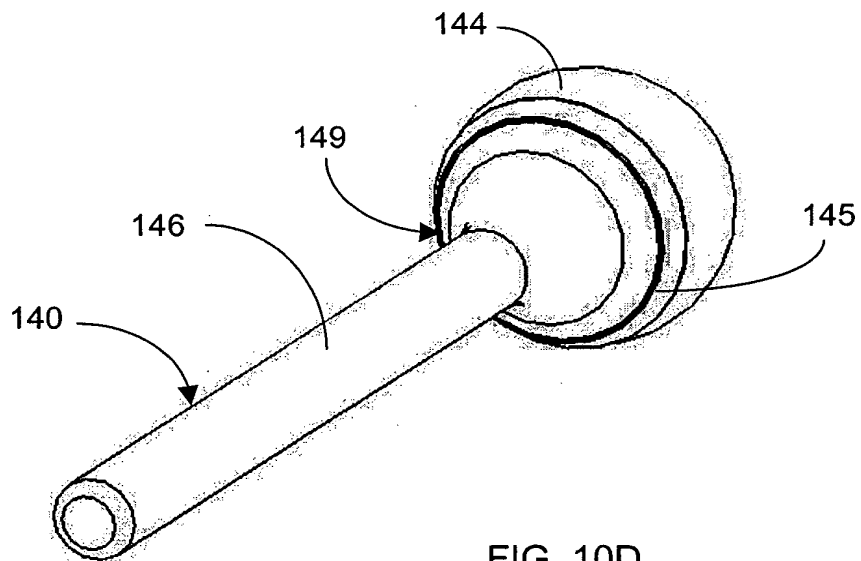


FIG. 10D

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown      Atty Docket: DEXCOM.011A

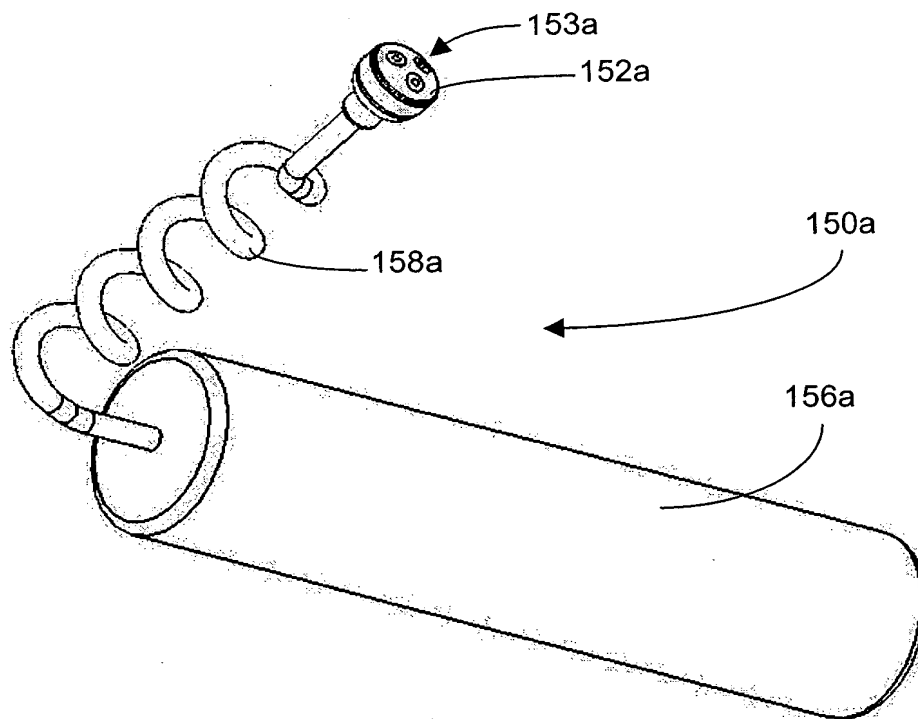


FIG. 11A

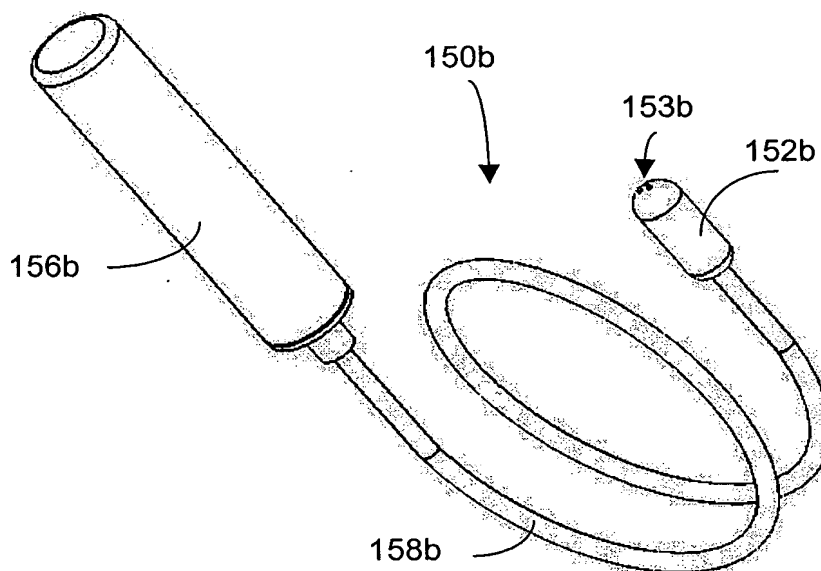


FIG. 11B

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.011A

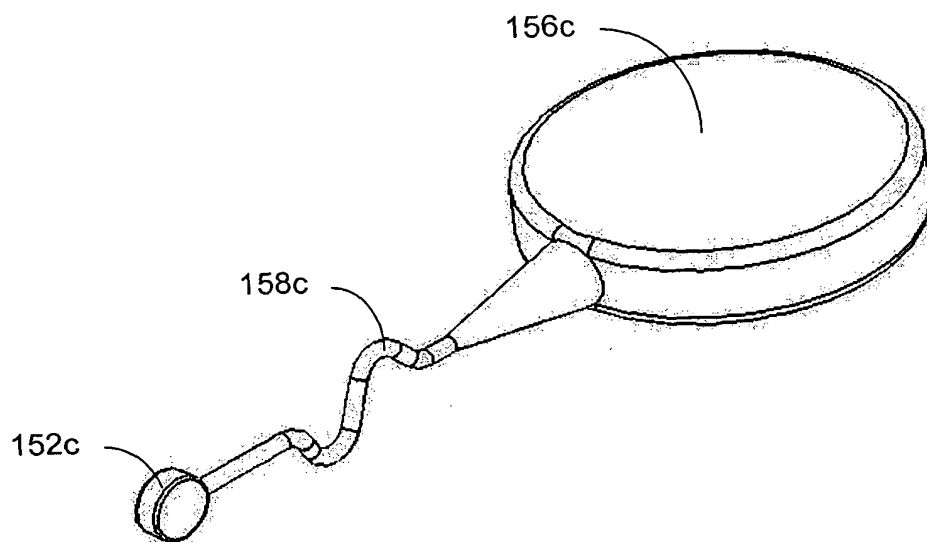


FIG. 11C

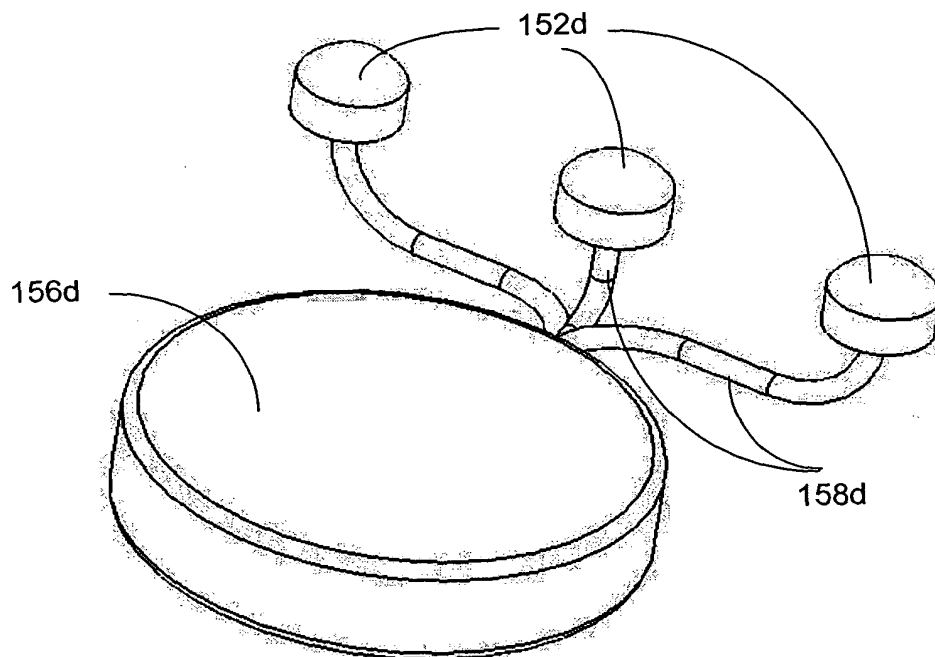


FIG. 11D

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.011A

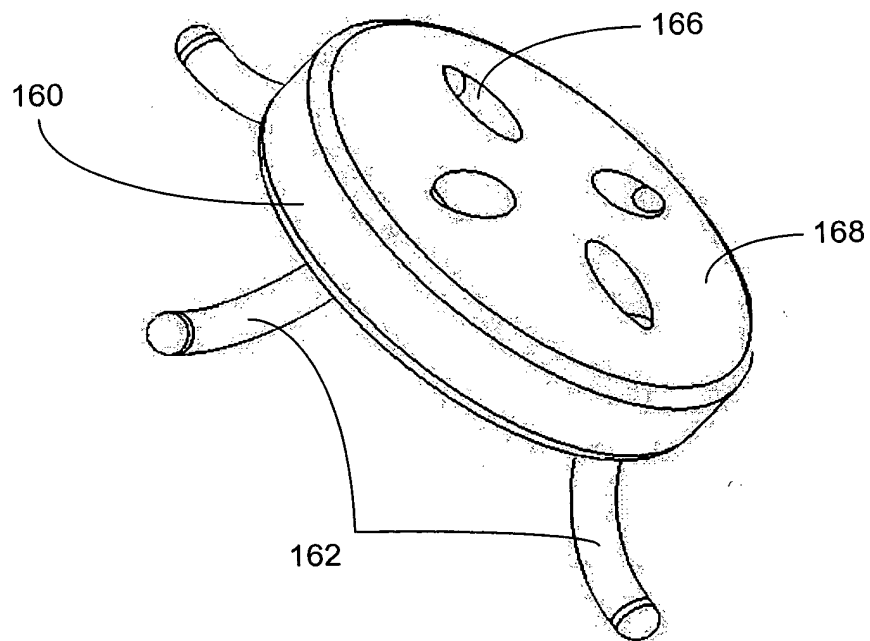


FIG. 12A

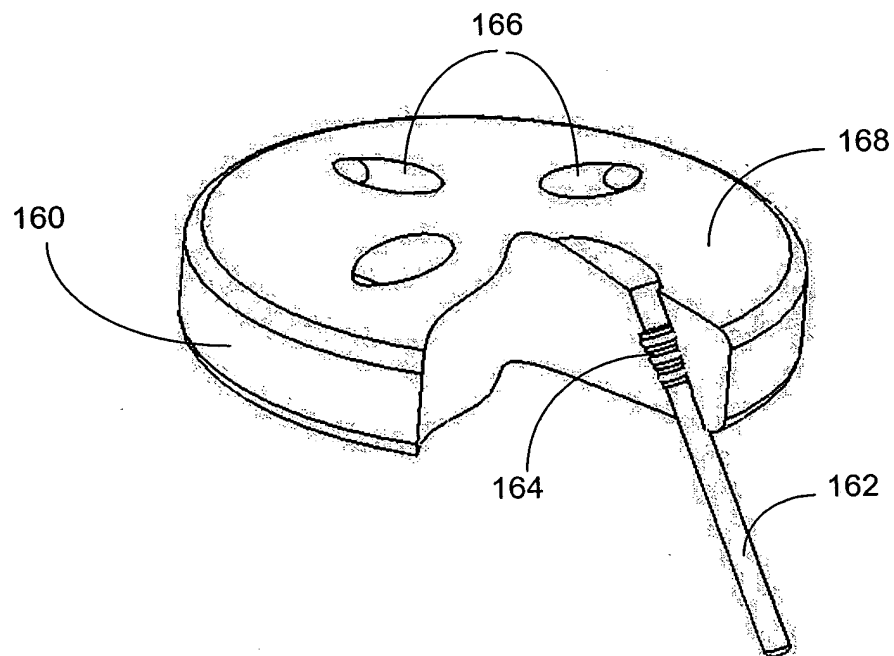


FIG. 12B

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.011A

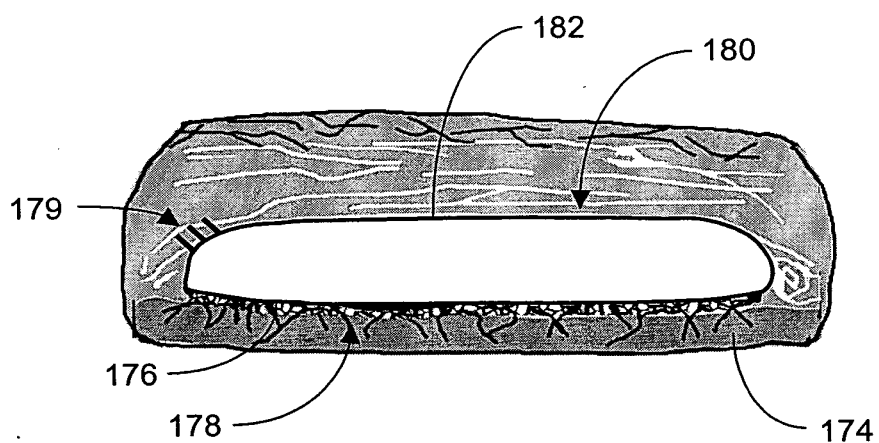
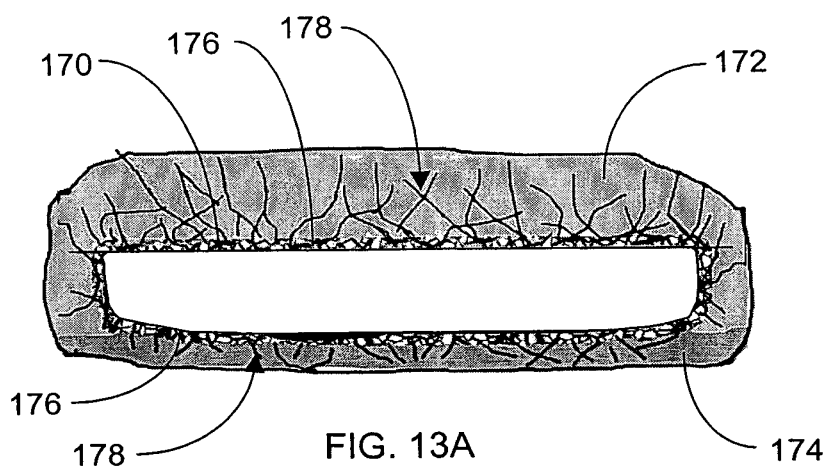


FIG. 13B

OPTIMIZED SENSOR GEOMETRY FOR AN IMPLANTABLE  
GLUCOSE SENSOR

Brauker, et al.

Appl. No.: Unknown Atty Docket: DEXCOM.011A

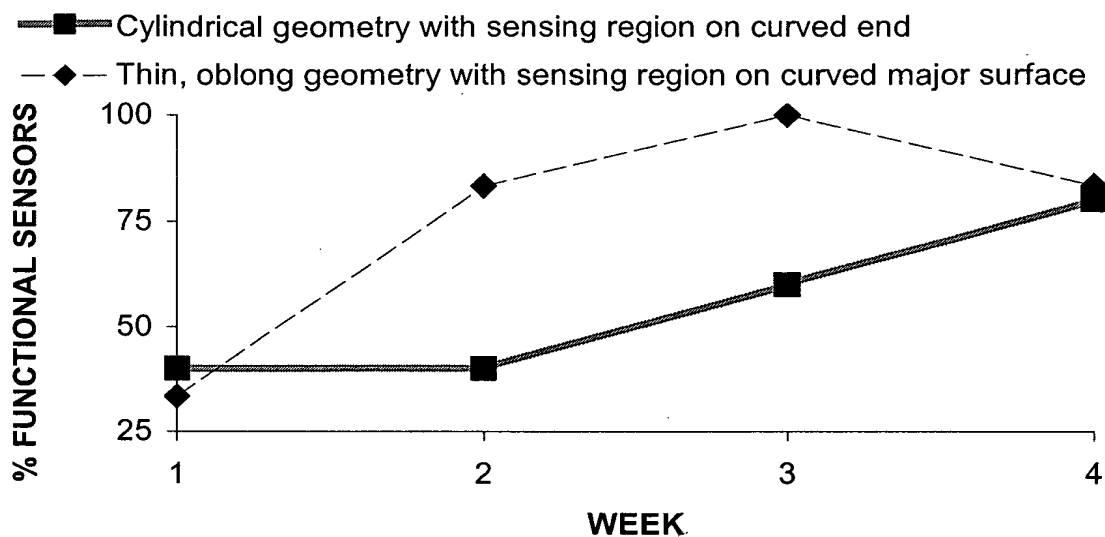


FIG. 14A

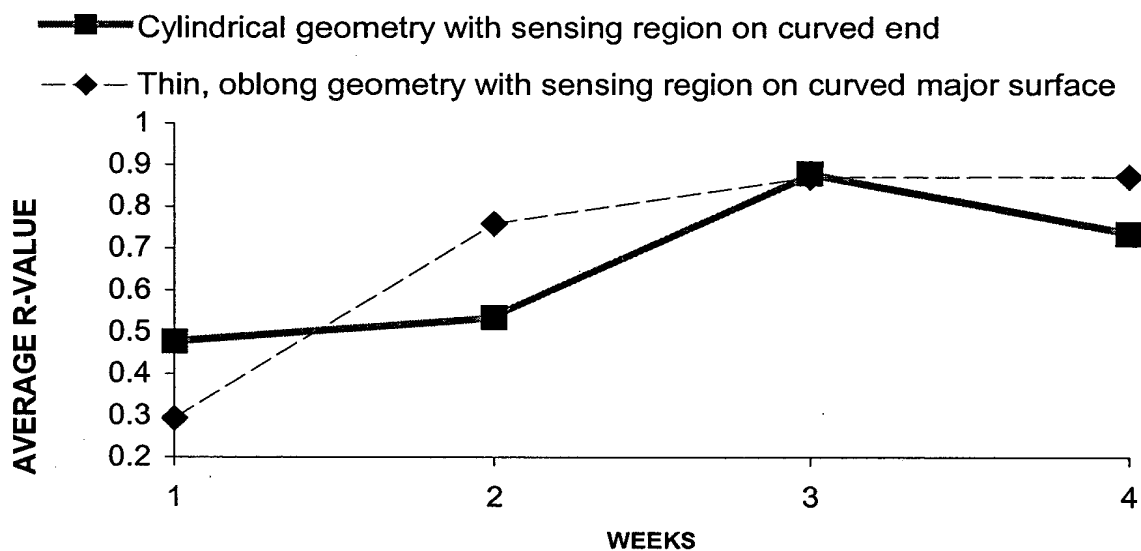


FIG. 14B